



DEPARTMENT OF HEALTH & HUMAN SERVICES

Public Health Service

Food and Drug Administration  
10903 New Hampshire Avenue  
Document Control Room -WO66-G609  
Silver Spring, MD 20993-0002

SeaSpine, Inc.  
% Mr. Dan Miller  
VP of Regulatory Affairs/CA & QA  
2301 La Mirada Drive  
Vista, California 92081

MAY 12 2011

Re: K102026

Trade/Device Name: SeaSpine Spacer System – Hollywood NM™ (Nanometalene™)  
Regulation Number: 21 CFR 888.3080  
Regulation Name: Intervertebral body fusion device  
Regulatory Class: Class II  
Product Code: MAX, MQP  
Dated: May 2, 2011  
Received: May 3, 2011

Dear Mr. Miller:

We have reviewed your Section 510(k) premarket notification of intent to market the device referenced above and have determined the device is substantially equivalent (for the indications for use stated in the enclosure) to legally marketed predicate devices marketed in interstate commerce prior to May 28, 1976, the enactment date of the Medical Device Amendments, or to devices that have been reclassified in accordance with the provisions of the Federal Food, Drug, and Cosmetic Act (Act) that do not require approval of a premarket approval application (PMA). You may, therefore, market the device, subject to the general controls provisions of the Act. The general controls provisions of the Act include requirements for annual registration, listing of devices, good manufacturing practice, labeling, and prohibitions against misbranding and adulteration. Please note: CDRH does not evaluate information related to contract liability warranties. We remind you; however, that device labeling must be truthful and not misleading.

If your device is classified (see above) into either class II (Special Controls) or class III (PMA), it may be subject to additional controls. Existing major regulations affecting your device can be found in the Code of Federal Regulations, Title 21, Parts 800 to 898. In addition, FDA may publish further announcements concerning your device in the Federal Register.

Please be advised that FDA's issuance of a substantial equivalence determination does not mean that FDA has made a determination that your device complies with other requirements of the Act


Page 2 – Mr. Dan Miller

or any Federal statutes and regulations administered by other Federal agencies. You must comply with all the Act's requirements, including, but not limited to: registration and listing (21 CFR Part 807); labeling (21 CFR Part 801); medical device reporting (reporting of medical device-related adverse events) (21 CFR 803); good manufacturing practice requirements as set forth in the quality systems (QS) regulation (21 CFR Part 820); and if applicable, the electronic product radiation control provisions (Sections 531-542 of the Act); 21 CFR 1000-1050.

If you desire specific advice for your device on our labeling regulation (21 CFR Part 801), please go to <http://www.fda.gov/AboutFDA/CentersOffices/CDRH/CDRHOffices/ucm115809.htm> for the Center for Devices and Radiological Health's (CDRH's) Office of Compliance. Also, please note the regulation entitled, "Misbranding by reference to premarket notification" (21 CFR Part 807.97). For questions regarding the reporting of adverse events under the MDR regulation (21 CFR Part 803), please go to <http://www.fda.gov/MedicalDevices/Safety/ReportaProblem/default.htm> for the CDRH's Office of Surveillance and Biometrics/Division of Postmarket Surveillance.

You may obtain other general information on your responsibilities under the Act from the Division of Small Manufacturers, International and Consumer Assistance at its toll-free number (800) 638-2041 or (301) 796-7100 or at its Internet address <http://www.fda.gov/MedicalDevices/ResourcesforYou/Industry/default.htm>.

Sincerely yours,

A handwritten signature in black ink, appearing to read "Mark N. Melkerson", with a stylized flourish at the end.

Mark N. Melkerson  
Director  
Division of Surgical, Orthopedic  
And Restorative Devices  
Office of Device Evaluation  
Center for Devices and  
Radiological Health

Enclosure

**Indications for Use**

**510(k) Number (if known):** K102026

**Device Name:** SeaSpine Spacer System - Hollywood NM™ (Nanometalene™)

**Indications for Use:**

When used as an intervertebral body fusion device, the SeaSpine Spacer System is intended for spinal fusion procedures at one or two contiguous levels (L2-S1) in skeletally mature patients with degenerative disc disease (DDD). DDD is defined as back pain of discogenic origin with degeneration of the disc confirmed by history and radiographic studies. DDD patients may also have up to Grade 1 spondylolisthesis or retrolisthesis at the involved level(s). These patients may have had a previous non-fusion spinal surgery at the involved spinal level(s). These patients should have had six months of non-operative treatment. The device is intended to be used with autogenous bone graft (autograft) and supplemental fixation.

When used as a vertebral body replacement device (VBR), the SeaSpine Spacer System is intended for use in the thoracolumbar spine (T1 to L5) to replace a collapsed, diseased, damaged or unstable complete or partial vertebral body due to tumor or trauma/fracture, to achieve anterior decompression of the spinal cord and neural tissues, and to restore the height of a collapsed vertebral body. The SeaSpine Spacer System is designed to restore the biomechanical integrity of the anterior, middle, and posterior spinal column, even in the absence of fusion for a prolonged period. Additionally, the device is intended for use with bone graft.

Prescription Use   X    
(Part 21 CFR 801 Subpart D)

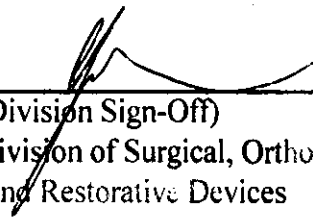
AND/OR

Over-The-Counter Use \_\_\_\_\_  
(21 CFR 801 Subpart C)

(PLEASE DO NOT WRITE BELOW THIS LINE-CONTINUE ON ANOTHER PAGE OF NEEDED)

---

Concurrence of CDRH, Office of Device Evaluation (ODE)

  
\_\_\_\_\_  
(Division Sign-Off)  
Division of Surgical, Orthopedic,  
and Restorative Devices

510(k) Number   K102026